SLIMLINE HANDLE

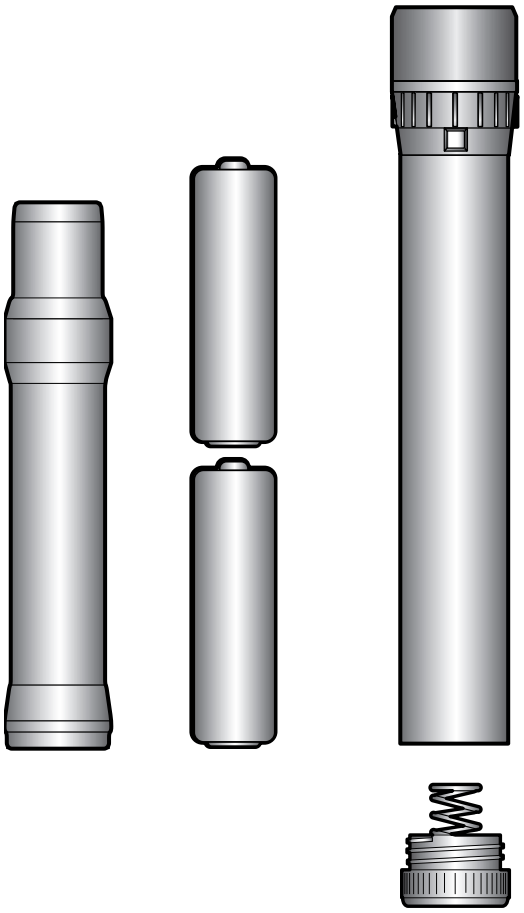

PLEASE READ AND FOLLOW THESE INSTRUCTIONS CAREFULLY

Keeler

Keeler Slimline Handles
Carefully read this Instruction Section before using your Keeler product. For your own safety and that of your customers observe all cautionary information provided in this section. The following information is intended to highlight potential safety hazards that can be associated with misuse, or damage.

Warning

This product must not be used in the presence of flammable gases.

Do not disassemble or modify the battery. There are no serviceable parts inside.

Do not dispose of battery in fire, Do not puncture.

Do not use a battery that is deformed, leaking, corroded or visually damaged.

If the product emits a strange odour, heat, or smoke, stop use immediately. The continued use of a damaged product or part may cause injuries.

Do not immerse the unit in any liquid

Do not use unit if damaged and periodically visually inspect for signs of damage.

Only Keeler Slimline handles with a red base can be used in the Keeler Lithium Charger. Do not try to insert a Keeler handle with a blue base into the Keeler Lithium Chargers. Refer to Keeler handle and bulb identification.

Caution
Remove dry cell batteries before prolonged periods of storage.

Use only Keeler rechargeable battery Pt. No. EP39 18918

Charge only using Keeler chargers Pt. Nos 1941-P-5289, Double Charger 1941-P-5326, Mini Charger

Do not mix battery types.

Do not charge battery in any environment where the temperature may exceed 40^{o}C or fall below 0^{o}C.

Keep out of reach of children.

For indoor use only (protect from moisture)

To prevent condensation from forming, allow instrument to come to room temperature before use.

When connecting instrument heads to handles check that voltage of the bulb in the instrument corresponds with the voltage of the handle.
Ensure that the control is in the off position when the examination has been completed.

When replacing Lithium cell, turn handle off and insert new cell. Replace bottom cap, and place handle into charging well.

Environmental
Dispose of battery in line with local regulations on recycling of batteries.

Tape over battery contacts to avoid short circuiting during disposal.

Li-ion batteries contain no toxic heavy metals, such as mercury, cadmium or lead.

Keeler Handle & Bulb Identification
Keeler handles & bulbs are colour coded to allow you to distinguish between a dry cell battery handle (2.8V) and a rechargeable handle (3.6v). The handles are colour coded as follows:

Blue Base = 2.8v for dry cell batteries
Red Base = 3.6v for rechargeable batteries

Please ensure when replacing bulbs that the voltage corresponds to the handle voltage.

Inserting/Replacing Batteries
Unscrew battery cap, insert batteries and replace battery cap as shown in Fig 1.

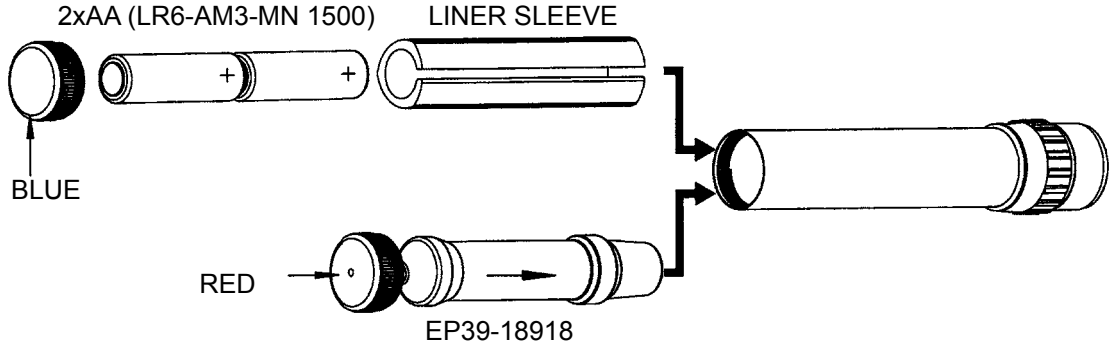

Fig. 1



Connection of the instrument heads to the handle.
The connection between the instrument head to the handle is a screw thread. To connect our instrument head connect as shown and rotate in clockwise direction. Ensure the connection between the head and handle is positive.



OFF

Compatibility
The Keeler Specialist, Professional, Standard and Practitioner Ophthalmoscopes and Keeler Retinoscopes are compatible with Keeler 2.8v and 3.6v Keeler handles.


HALF ON

On/Off brightness control
To switch the instrument on, rotate the brightness control as indicated to the right.
To switch off the instrument, rotate the brightness control as indicated to the left.
Keeler Slimline Handles have a power indicator. This will show if the instrument is on or off.
Red = on Silver = off.


FULL ON

Handle Identification
Keeler Slimline and pocket handles are colour coded to allow you to distinguish between a dry cell battery handle (2.8v) and a rechargeable handle (3.6v). The handles are colour coded as follows:
Blue base = 2.8v. for dry cell batteries (with sleeve liner.) 13A
Red base = 3.6v for rechargeable batteries. 13B

Cleaning Instructions
Only manual non-immersion cleaning as described below should be used for the instrument:

1. Wipe the external surface with a clean absorbent, non shedding cloth dampened with a water / detergent solution (2% by volume) or water / isopropyl alcohol solution (70% by volume).

2. Ensure that excess solution does not enter the instrument. Use caution to ensure cloth is not saturated with solution.

3. Surfaces should be carefully hand-dried using a clean non-shedding cloth.

4. Safely dispose of used cleaning materials.

Warranty & Service
No user serviceable parts - all preventative maintenance and servicing must only be performed by authorised Keeler representatives.

Your Keeler handle is guaranteed for 3 years and will be replaced or repaired free of charge subject to the following:

1. Any fault is due to faulty manufacture
2. Proof of purchase accompanies any claim.

MANUFACTURED IN THE UK BY:

Keeler Limited
Clewer Hill Road
Windsor
Berkshire SL4 4AA
England
Tel: +44 (0)1753 857177
Fax: +44 (0)1753 827145
FREEPHONE: 0800 521 251

Distributed by:

Keeler Instruments Inc
456 Parkway
Broomall
PA 19008, USA
Toll Free: 1 800 523 5620
Tel: 610 353 4350
Fax: 610 353 7814

The CE mark on this product indicates it has been tested to and conforms with the provisions noted within the 93/42/eec Medical Device Directive.

A HALMA GROUP COMPANY

Distributor